

# Exploring the bq20z80 Impedance Track™ Evaluation Kit

Doug Williams

Battery Management

## ABSTRACT

The bq20z80 evaluation module (EVM) and its corresponding evaluation software provides a rich and effective environment for examining the bq20z80 – a new, advanced battery gas gauge. This application report covers this EVM and software with an emphasis on how to use it and what to expect. EVM board connections are discussed in detail, and helpful hints are offered. For the evaluation software, components of each major screen are presented along with the various menu options.

## Contents

1	Connecting the EVM .....	1
2	Scanning the SBS Registers .....	3
3	Logging the SBS Registers.....	4
4	Editing the Data Flash .....	5
5	Calibrating the bq20z80 .....	7
6	The Pro Screen .....	8
7	EVM Schematic .....	10


## List of Figures

1	EVM Connections .....	2
2	All Flags and Status Bits Are Visible on a 1024x768 Screen if the Top Display Buttons Are Hidden.....	3
3	Vertically Tiled View of SBS, Data Flash, and Pro Screen .....	4
4	Example of bq20z80 Data Flash Organization. 1 <sup>st</sup> Level Safety Class of Data Flash Constants. Subclasses are Voltage, Current, Temperature, and Host Comm. ....	6
5	Five Steps to Force the Remaining Capacity to 1000 mAh.....	9

## 1 Connecting the EVM

The cell-connection terminal blocks provide screw terminals for connecting 2, 3, or 4 cells to the evaluation module (EVM). The numbering convention for batteries is that Cell 1 is the most negative; so, connect the 1N (N=negative) terminal on the EVM to the most negative point of your battery stack.

If evaluating a 3-cell application, connect both 3P and 4P (P = positive) to the top node of the cell stack. Similarly, for a 2-cell application, connect 2P, 3P, and 4P to the top node.

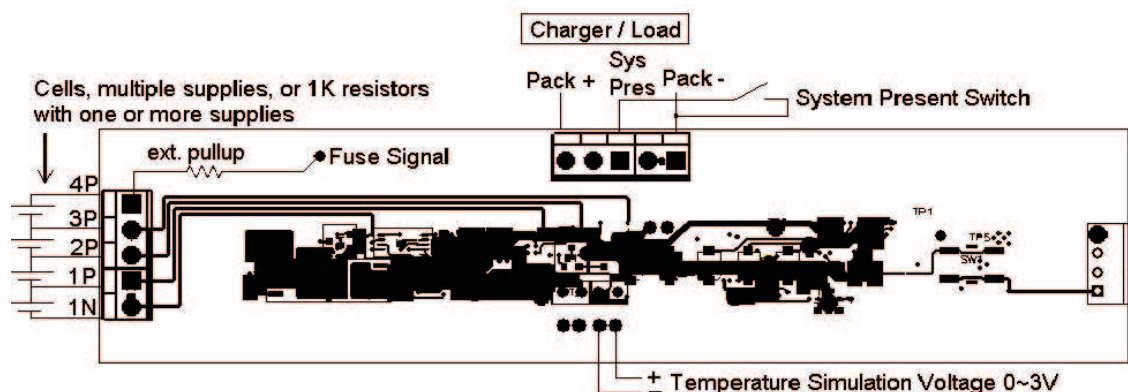

**Figure 1. EVM Connections**

### 1.1 Cells, Resistors, or Power Supplies?

For quick evaluation of the bq20z80 safety features, using real cells can be a burden. Therefore, substitute a string of 1-k $\Omega$  resistors fed with a single laboratory power supply. The supply can be varied quickly to investigate pack voltage protection. An additional floating supply can be connected across one of the resistors to simulate cell over- and undervoltages.

However, be aware that the Impedance Track™ algorithm, which relies on measuring the actual cell impedance, does not operate correctly without real cells.

### 1.2 Where is the Fuse?

The EVM does not include the chemical fuse that is employed in many battery pack applications. This eliminates the need for fuse replacement when running fault tests. Instead, the signal on TP4 shows the control that would blow the fuse. It requires an external pullup resistor to the battery voltage in order to monitor its state on a scope or meter

### 1.3 System Present and Pack Connections

The Pack+ and Pack– connections are used to connect the load and charger. It may be convenient to simultaneously connect a laboratory power supply and an electronic load in parallel. Most electronic loads have a load on/off switch and adjusting the constant current limit control to zero can disable the laboratory power supply.

### 1.4 Simulating Current

If using a string of resistors to simulate cells, it is difficult to apply an actual charge current. The solution is to connect a floating laboratory power supply between Pack– and Battery– (1N). Putting the floating supply in current limit provides a simulated charge current that is forced through the sense resistor. Depending on the laboratory power supplies available, this configuration can be useful for load current by reversing the polarity of the current source connections. Use this configuration to quickly test various overcurrent safety features or to validate coulomb counting accuracy. However, be aware that this method bypasses the protection FETs, and fault conditions will not interrupt the charge or load current.

### 1.5 Simulating Temperature

Because the temperature measurement works by measuring the voltage on the thermistor pin, a temperature chamber for safety evaluation is unnecessary. Just connect a laboratory power supply across the RT1 terminals with the positive output on X3 (see the EVM schematic located at the end of this document). In this case, this power supply does not have to be isolated from the supply used to simulate a charger/load because the return side of the thermistor is the same as Pack–. Forcing 0 V ~ 3 V across the thermistor allows testing the safety features over the full temperature range.

## 2 Scanning the SBS Registers

With the battery connections made, start the evaluation software. When first connected, the circuitry may be in shutdown mode. This normally requires applying a charging source across the Pack+ and Pack- terminals. If a charger voltage is not connected, briefly connect the positive battery voltage to Pack+.

### 2.1 Setting the Scan Interval

By default, the SBS register scanning is off. Put a check in the *Keep Scanning* box to get the scanning started. A periodic update of all the SBS registers should appear. Note the blue progress bar at the bottom. The interval between scans can be set in the Options | Set Scan Interval menu. The program remembers this setting and uses it each time the program is launched.

### 2.2 Adjusting the View

With some screen resolutions, it may not be possible to see all of the register displays simultaneously. In some cases, this can be improved by making the top buttons invisible. Use the View | Display Buttons menu to remove these objects from the screen (see Figure 2).

The Evaluation Software, EVSW, has the flexibility to allow multiple views. Two or three screens can be tiled onto the display at once. After opening any of the SBS, Data Flash, or Pro screens, use the Window menu to tile them either vertically or horizontally. Figure 3 shows a vertically tiled view of all three.

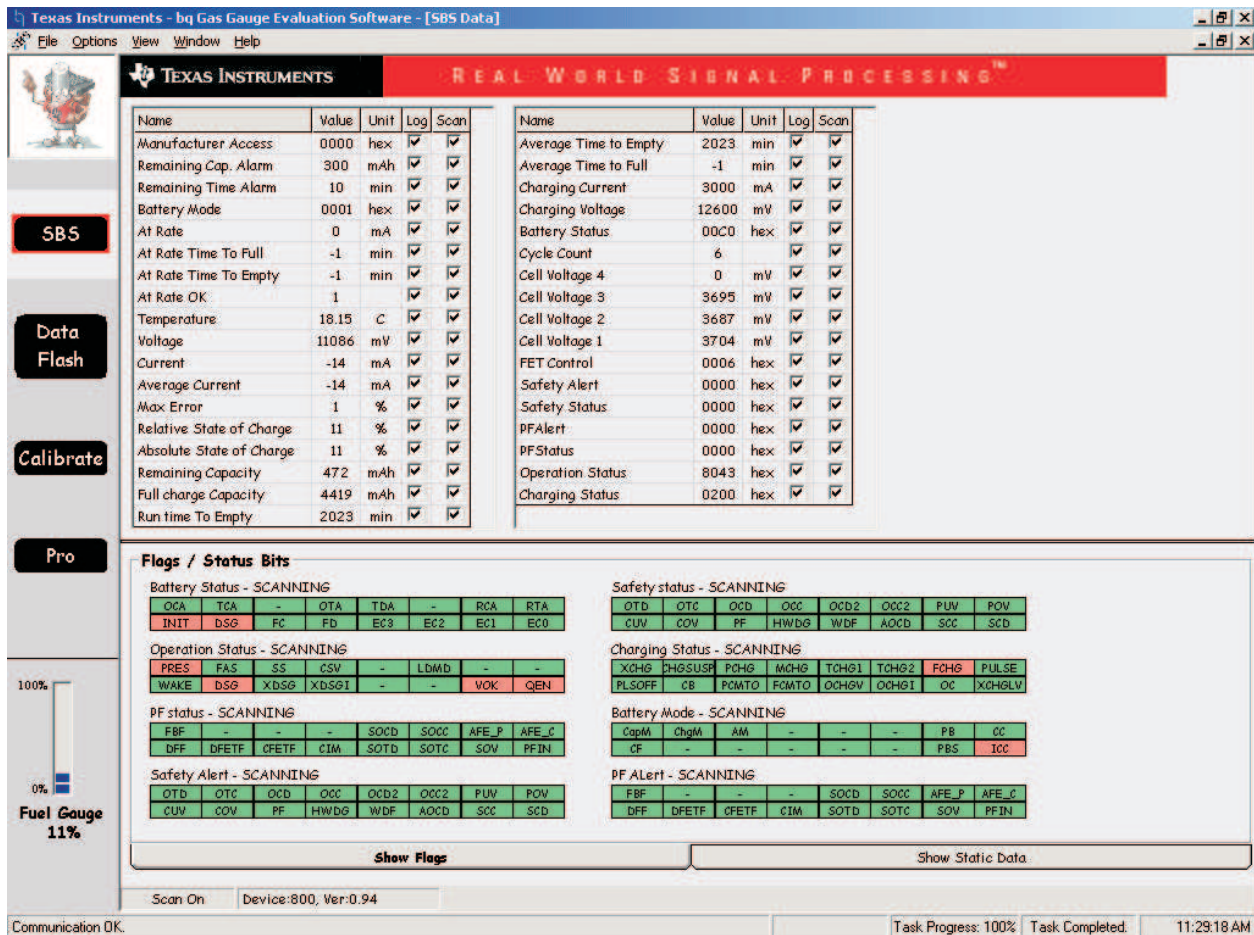


Figure 2. All Flags and Status Bits Are Visible on a 1024x768 Screen if the Top Display Buttons Are Hidden

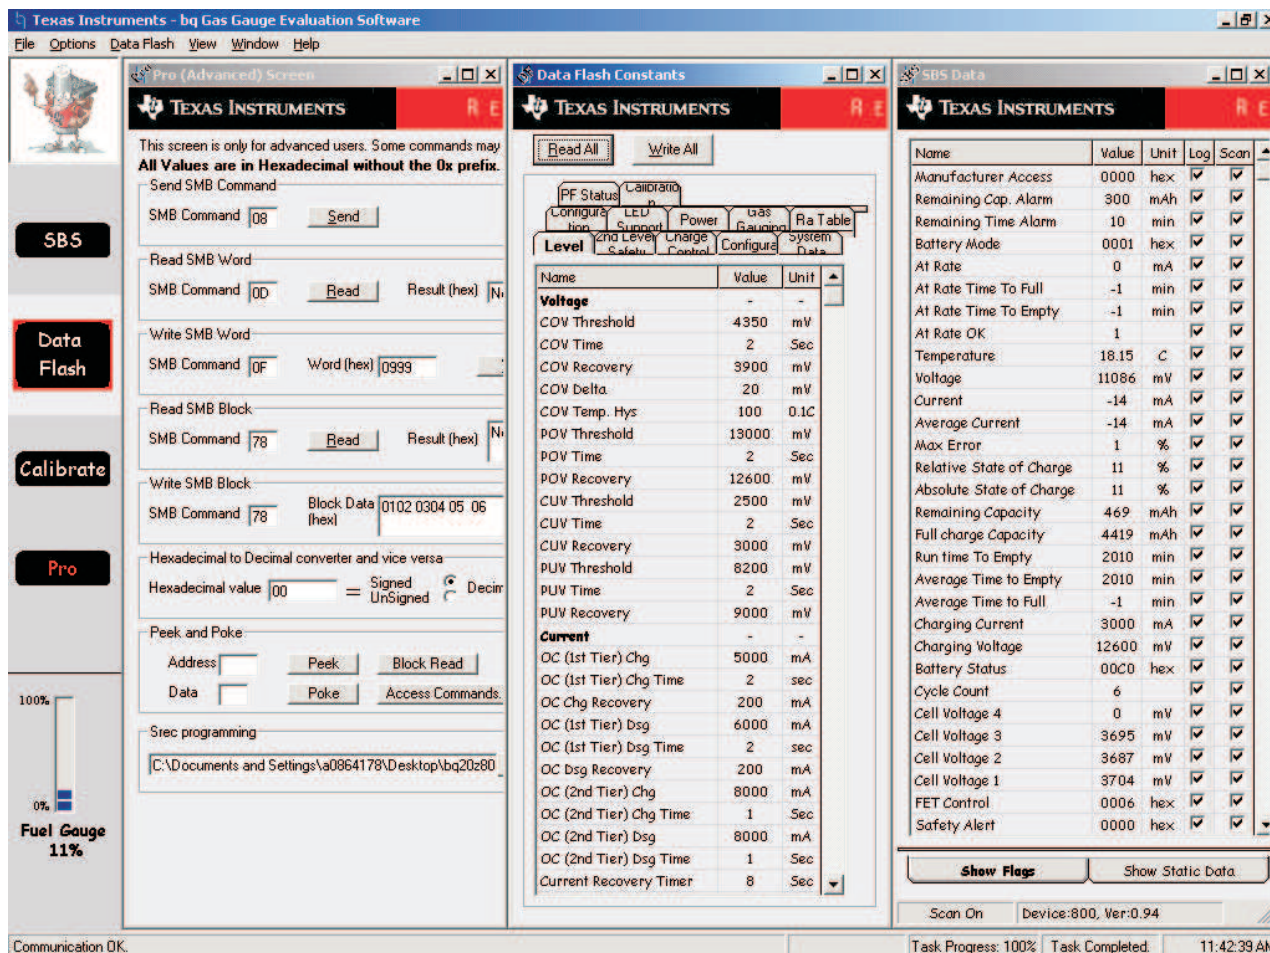


Figure 3. Vertically Tiled View of SBS, Data Flash, and Pro Screen

### 2.3 Flags / Status Bits

The flags and status bit displays are bit expansions of the various status, alert, and battery mode registers. The red bit cells are asserted, whereas the green cells are not. The displayed mnemonics are an improvement compared to decoding hexadecimal digits, but consult the data sheet to learn the full definition for each bit.

## 3 Logging the SBS Registers

Due to the long time associated with battery testing, it is common to data-log complete charge and discharge cycles for later analysis. When evaluating a new cell type, or a new gas gauge device, logs provide a convenient and effective way to understand the process.

### 3.1 Configuring the Log File

The log file can be configured to record any combination of the displayed SBS and extended registers. Simply check or uncheck the items to log. Select or deselect all of them quickly using the Options menu. It is usually a good idea to deselect the registers that are not relevant to the experiment being performed in order to simplify the process of reading the log later and to reduce the size of the log file.

The logging interval is also configured from a dialog box available in the options menu. Consider the purpose for the log when choosing an interval. If you expect to see several events during a short period, or are looking for a transient phenomenon, then a short interval, such as 1000 milliseconds can be used. This produces a huge file when run overnight, so decrease the resolution if it is not really necessary.

Start and stop the logging process with the buttons near the top of the screen. The state of the Start Logging and Stop Logging buttons immediately reveal if the program is logging or not.

### **3.2 Using Excel for Log File Evaluation**

The log file is written as records of tab delimited ASCII. This file format can be imported into Microsoft™ Excel without any extra steps. Just right-click on the file name, and select Open With | Microsoft Excel for Windows™. However, one problem that can arise is with columns containing hexadecimal values. If the data contains an "e", Excel interprets this as scientific notation by default. If this situation occurs, use the import function in Excel, and modify the column type for the target column to be "text."

Microsoft Excel has a function in its Window menu called Freeze Panes, which is extremely helpful for reviewing long lists of records. Highlight the first row of data, under the heading row, and choose Freeze Panes from the Window menu. Now you can scroll through the entire log and still see the heading for each column. Sometimes, it is more convenient to delete the header information in lines 1 through 11.


## **4 Editing the Data Flash**

The data flash screen displays the classes and subclasses used to categorize the data flash constants. The classes are on the index tabs at the top. Select a tab to activate the display for all the constants within that class. The 12 data flash constant classes are 1st Level Safety, 2nd Level Safety, Charge Control, Gas Gauging, SBS Configuration, Ra Table, Pf Status, Calibration, System Data, Configuration, LED Support, and Power. Each constant is described in the application report *Configuring the bq20z80 Data Flash* ([SLUA342](#)).

### **4.1 Navigating the Data Flash – Classes and Subclasses**

The classes of constants are selected with the tabs; under each class are also subclass groupings . For example, click on the 1st Level Safety Tab. Shown in the grids are the various data flash constants with subclass indicators in bold type. In this case, the subclasses are Voltage, Current, Temperature, and Host Comm.

## Editing the Data Flash

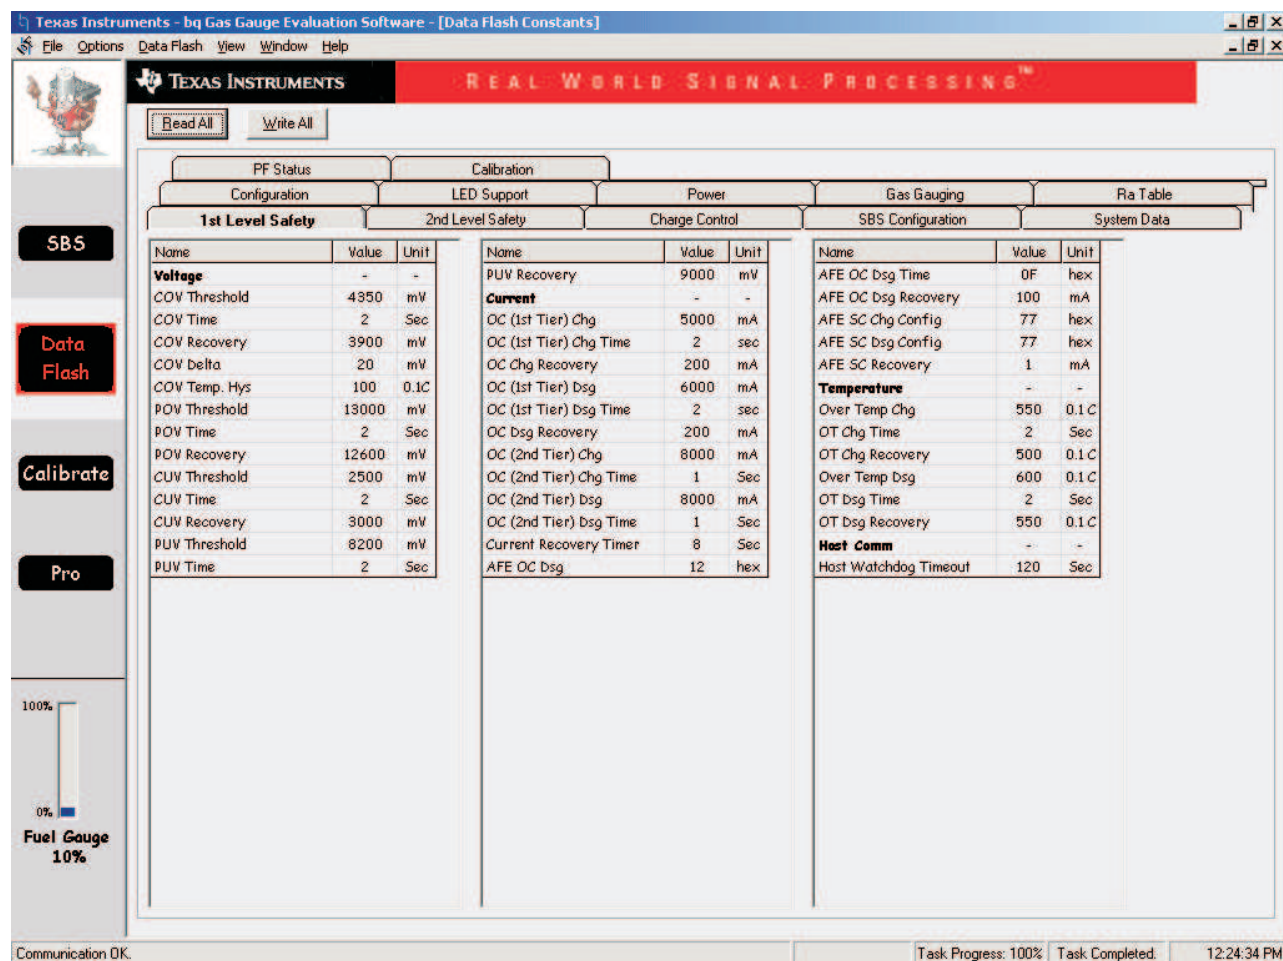

Texas Instruments - bq Gas Gauge Evaluation Software - [Data Flash Constants]

File Options Data Flash View Window Help

TEXAS INSTRUMENTS REAL WORLD SIGNAL PROCESSING™

Read All Write All

SBS

Data Flash

Calibrate

Pro

Fuel Gauge 10%

1st Level Safety			2nd Level Safety			Charge Control			SBS Configuration			System Data		
Name	Value	Unit	Name	Value	Unit	Name	Value	Unit	Name	Value	Unit	Name	Value	Unit
<b>Voltage</b>	-	-	PUV Recovery	9000	mV	AFE OC Dsg Time	0F	hex	AFE OC Dsg Recovery	100	mA	AFE SC Chg Config	77	hex
COV Threshold	4350	mV	<b>Current</b>	-	-	AFE SC Chg Config	77	hex	AFE SC Dsg Config	77	hex	AFE SC Recovery	1	mA
COV Time	2	Sec	OC (1st Tier) Chg	5000	mA	<b>Temperature</b>	-	-	Over Temp Chg	550	0.1 C	OT Chg Time	2	Sec
COV Recovery	3900	mV	OC (1st Tier) Chg Time	2	sec	Over Temp Dsg	600	0.1 C	OT Dsg Time	2	Sec	OT Dsg Recovery	550	0.1 C
COV Delta	20	mV	OC Chg Recovery	200	mA	OT Chg Recovery	500	0.1 C	Current Recovery Timer	8	Sec	Host Comm	-	-
COV Temp. Hys	100	0.1C	OC (1st Tier) Dsg	6000	mA	Host Watchdog Timeout	120	Sec						
POV Threshold	13000	mV	OC (1st Tier) Dsg Time	2	sec									
POV Time	2	Sec	OC Dsg Recovery	200	mA									
POV Recovery	12600	mV	OC (1st Tier) Chg	8000	mA									
CUV Threshold	2500	mV	OC (2nd Tier) Chg Time	1	Sec									
CUV Time	2	Sec	OC (2nd Tier) Dsg	8000	mA									
CUV Recovery	3000	mV	OC (2nd Tier) Dsg Time	1	Sec									
PUV Threshold	8200	mV	Current Recovery Timer	8	Sec									
PUV Time	2	Sec	AFE OC Dsg	12	hex									

Communication OK. Task Progress: 100% Task Completed. 12:24:34 PM

Figure 4. Example of bq20z80 Data Flash Organization. 1<sup>st</sup> Level Safety Class of Data Flash Constants. Subclasses are Voltage, Current, Temperature, and Host Comm.

### 4.2 Reading and Editing Data Flash

Use the Read All button initially to populate the grids. Make a change to any constant in the value column, and press Enter to write the new value into the device data flash. Note that data cannot be written to the device if it is sealed or in a permanent fail state.

### 4.3 Exporting and Auto Export

A list of all the data flash values may be stored to a text file with a .gg extension. The format of this file includes the class, subclass, name, and value for each data flash location. For example:

- [Voltage(1st Level Safety)]
- COV Threshold = 4350
- COV Time = 2
- COV Recovery = 3900
- COV Delta = 20
- COV Temp. Hys = 100
- POV Threshold = 13000
- POV Time = 2
- POV Recovery = 12600

- CUV Threshold = 2500
- CUV Time = 2
- CUV Recovery = 3000
- PUV Threshold = 8200
- PUV Time = 2
- PUV Recovery = 9000

Note that the constants are grouped under subclass and class which are identified with a line of text in the format: [Subclass(Class)].

These files can be generated automatically at programmed intervals using the AutoExport feature. Use the Options menu to set the interval and the file name. Then, start the feature with the AutoExport menu command. At each programmed interval, a new .gg file is written, with an index number appended to the file name. This feature is useful for tracking data flash values that may change over time, such as the resistance values for each cell in the Ra Table.

#### **4.4 Importing and Writing All**

The .gg file can be saved and then imported into another device. Use the File | Import menu to select a .gg file. Doing this brings the data into the data flash grids, where it can be reviewed and edited. To transfer all the data into the bq20z80 gas gauge, push the Write All button.

### **5 Calibrating the bq20z80**

The calibration screen provides a flexible platform for device calibration of offsets, voltage, current, and temperature. The four common calibration functions and an optional pack voltage calibration and board offset calibration appear on this screen.

#### **5.1 CC Offset Calibration**

The coulomb current offset calibration is a prerequisite for voltage, temperature, and current gain calibrations, because a gain calibration with an offset present is not accurate. By default, this is a quick version of the offset calibration. A full calibration occurs each time the bq20z80 enters sleep mode. Although the various gain calibrations may be performed independently, the CC offset calibration must be performed at least once prior to use in order to correct for any CC offset error.

#### **5.2 Voltage and Temperature Calibration**

Enter the known value of voltage and temperature. Select the number of cells in the application. Select the type of temperature sensors used in the application.

#### **5.3 Current Calibration**

Enter the applied current, which should be approximately 2 A.

#### **5.4 Pack Voltage Calibration**

Pack voltage calibration is not generally necessary. This is used to calibrate a separate measurement path, which only detects if a charger is present.

#### **5.5 Board Offset Calibration**

Board offset calibration is not so much a calibration as it is a characterization of the current leakage errors and noise inherent in a given PCB design. The value should be found for a given design and then used for each board produced. For best accuracy, absolutely no current must flow through the sense resistor, including the current used to power the devices. That means that the bq29312 must be powered from the charger and not from the cells. The protection FETs are automatically opened during this procedure to ensure that the AFE is powered only from the pack input. Therefore, device current does not pass through the sense resistor.

## **6 The Pro Screen**

The Pro screen can be used to read and write low-level SMBus transactions, peek and poke the RAM of the bq20z80, and reprogram the bq20z80 flash memory. The write operations should not be done without understanding the implications.

### **6.1 SMB Commands, Words, and Blocks**

SMBus commands, words, and blocks can be easily read or written on the Pro screen. The most common use of this facility is to send 0x0021 to SMB command 0x00 (Manufacturer Access) in order to start the Impedance Track™ algorithm.

### **6.2 An Example – Modifying Remaining Capacity**

Some of the SMBus registers, even though specified as read only, can be written when the device is unsealed for evaluation purposes only. For example, Remaining Capacity is SMBus command 0x0F. Suppose that it is desired to force Remaining Capacity to be 1000 mAh. With reference to [Figure 5](#), the process involves the following five steps:

1. Use the hexadecimal-to-decimal calculator to determine the hexadecimal value of 1000 mAh. Enter 1000 in the decimal text box.
2. The hexadecimal equivalent displayed in the hexadecimal text box is 3E8.
3. Enter 03E8 in the SMB Write Word data text box
4. Enter the command 0F in the SMB Write Word command text box.
5. Press the Write button.



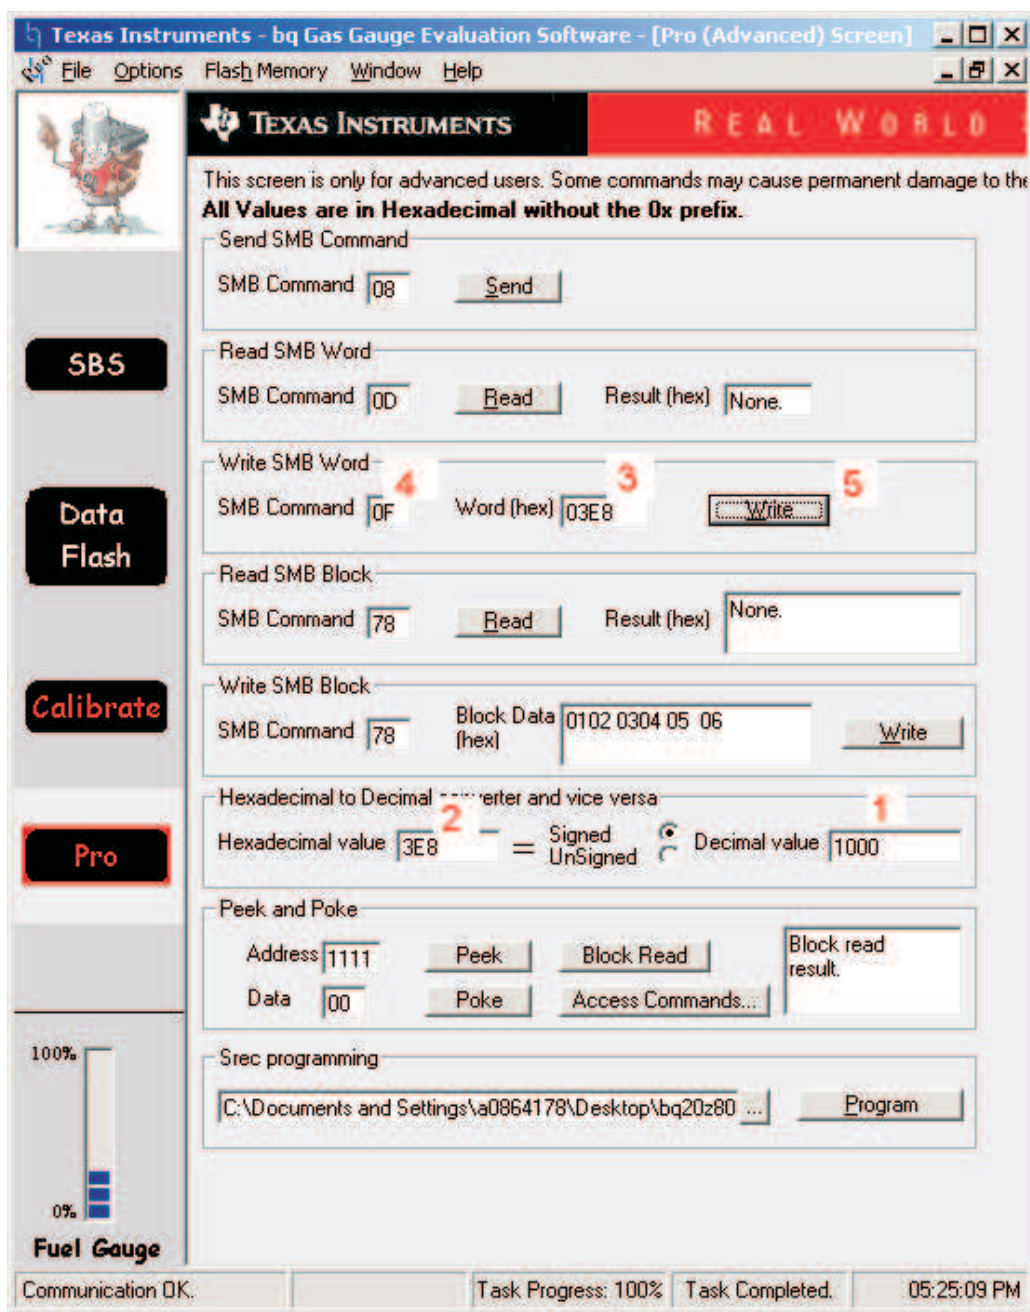


Figure 5. Five Steps to Force the Remaining Capacity to 1000 mAh

### 6.3 Peek and Poke

Use this feature only for advanced debugging with the guidance of TI engineers. The peek and poke feature may not be available in some versions of this program.

### 6.4 SREC Programming

Programming or *Re-flashing* the bq20z80 is also an advanced topic, which can be useful in certain circumstances. The object files used to program the device have the extension *.senc* which refers to an encrypted s-record.

**7 EVM Schematic**

The EVM schematic appears on the following page.

## IMPORTANT NOTICE

Texas Instruments Incorporated and its subsidiaries (TI) reserve the right to make corrections, modifications, enhancements, improvements, and other changes to its products and services at any time and to discontinue any product or service without notice. Customers should obtain the latest relevant information before placing orders and should verify that such information is current and complete. All products are sold subject to TI's terms and conditions of sale supplied at the time of order acknowledgment.

TI warrants performance of its hardware products to the specifications applicable at the time of sale in accordance with TI's standard warranty. Testing and other quality control techniques are used to the extent TI deems necessary to support this warranty. Except where mandated by government requirements, testing of all parameters of each product is not necessarily performed.

TI assumes no liability for applications assistance or customer product design. Customers are responsible for their products and applications using TI components. To minimize the risks associated with customer products and applications, customers should provide adequate design and operating safeguards.

TI does not warrant or represent that any license, either express or implied, is granted under any TI patent right, copyright, mask work right, or other TI intellectual property right relating to any combination, machine, or process in which TI products or services are used. Information published by TI regarding third-party products or services does not constitute a license from TI to use such products or services or a warranty or endorsement thereof. Use of such information may require a license from a third party under the patents or other intellectual property of the third party, or a license from TI under the patents or other intellectual property of TI.

Reproduction of information in TI data books or data sheets is permissible only if reproduction is without alteration and is accompanied by all associated warranties, conditions, limitations, and notices. Reproduction of this information with alteration is an unfair and deceptive business practice. TI is not responsible or liable for such altered documentation.

Resale of TI products or services with statements different from or beyond the parameters stated by TI for that product or service voids all express and any implied warranties for the associated TI product or service and is an unfair and deceptive business practice. TI is not responsible or liable for any such statements.

Following are URLs where you can obtain information on other Texas Instruments products and application solutions:

<b>Products</b>		<b>Applications</b>	
Amplifiers	<a href="http://amplifier.ti.com">amplifier.ti.com</a>	Audio	<a href="http://www.ti.com/audio">www.ti.com/audio</a>
Data Converters	<a href="http://dataconverter.ti.com">dataconverter.ti.com</a>	Automotive	<a href="http://www.ti.com/automotive">www.ti.com/automotive</a>
DSP	<a href="http://dsp.ti.com">dsp.ti.com</a>	Broadband	<a href="http://www.ti.com/broadband">www.ti.com/broadband</a>
Interface	<a href="http://interface.ti.com">interface.ti.com</a>	Digital Control	<a href="http://www.ti.com/digitalcontrol">www.ti.com/digitalcontrol</a>
Logic	<a href="http://logic.ti.com">logic.ti.com</a>	Military	<a href="http://www.ti.com/military">www.ti.com/military</a>
Power Mgmt	<a href="http://power.ti.com">power.ti.com</a>	Optical Networking	<a href="http://www.ti.com/opticalnetwork">www.ti.com/opticalnetwork</a>
Microcontrollers	<a href="http://microcontroller.ti.com">microcontroller.ti.com</a>	Security	<a href="http://www.ti.com/security">www.ti.com/security</a>
		Telephony	<a href="http://www.ti.com/telephony">www.ti.com/telephony</a>
		Video & Imaging	<a href="http://www.ti.com/video">www.ti.com/video</a>
		Wireless	<a href="http://www.ti.com/wireless">www.ti.com/wireless</a>

Mailing Address: Texas Instruments  
Post Office Box 655303 Dallas, Texas 75265